


# Syphilis Testing Algorithm

## Indications for Testing:

- Persons with signs or symptoms of syphilis infection
- Asymptomatic persons at high risk for syphilis (or of transmitting the disease to others)

## Testing Algorithm:

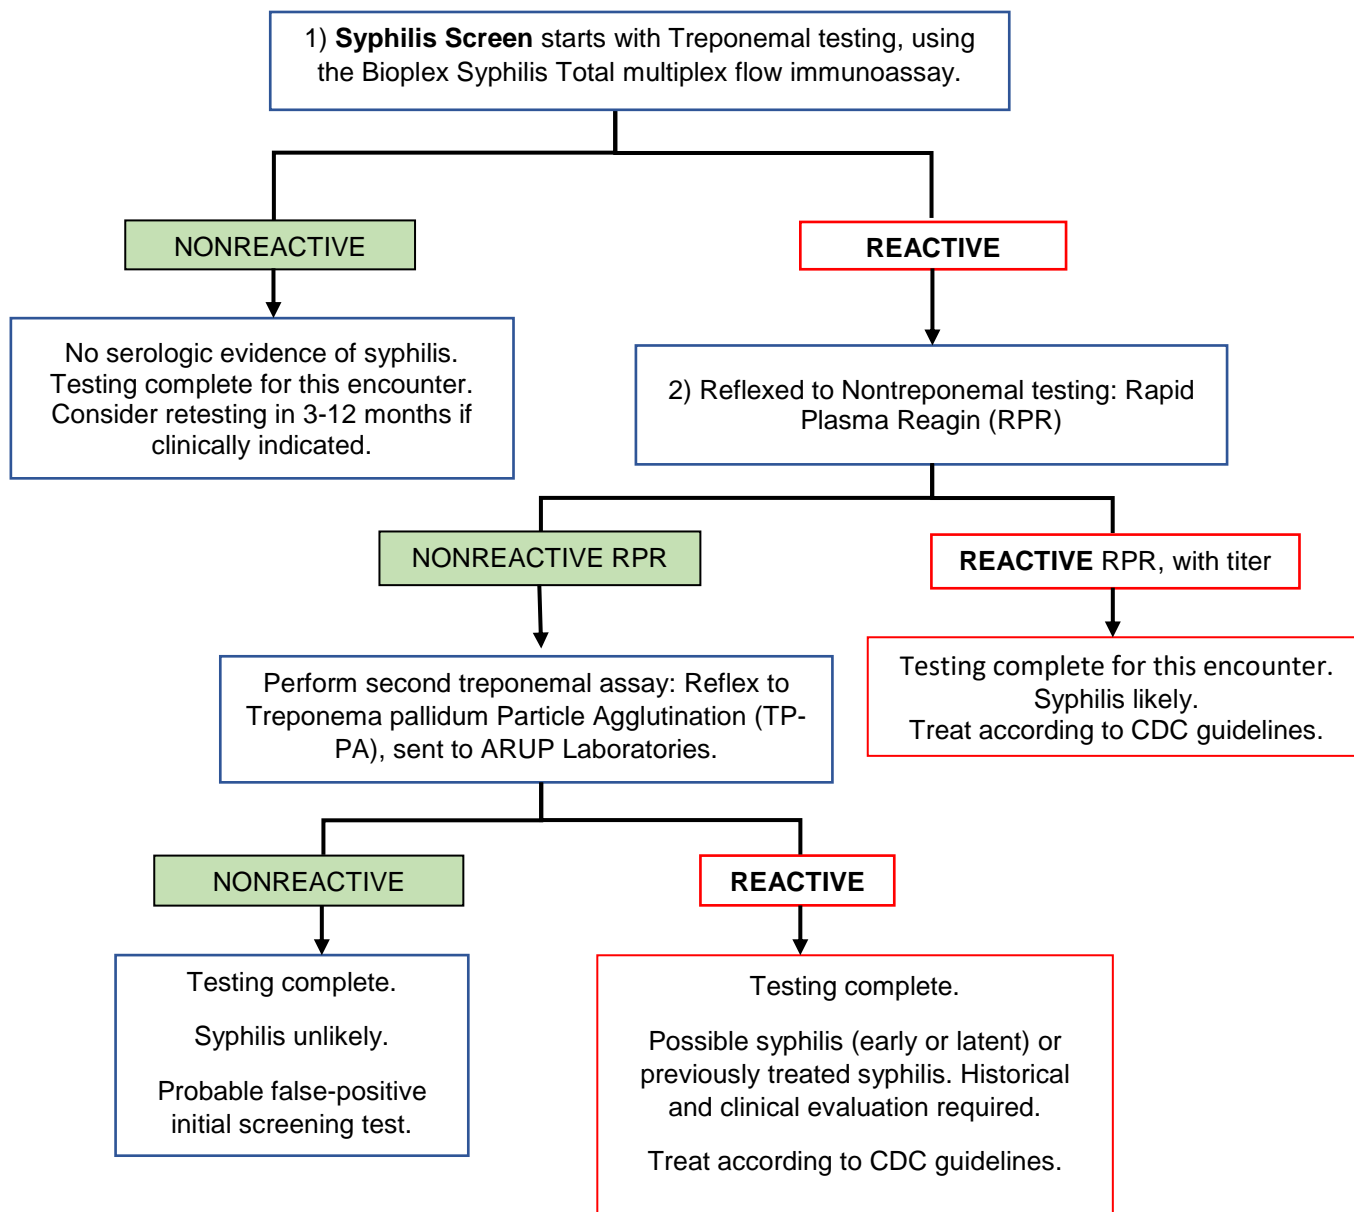

# Syphilis Testing Algorithm

## Reverse Sequence Screening Algorithm Explained:

As an alternative to the traditional syphilis screening algorithm, many laboratories utilize the reverse syphilis screening algorithm. This algorithm starts with an automated treponemal assay, such as an enzyme immunoassay and multiplex flow immunoassay (MFI), to detect antibodies specific to *T pallidum*. If the screening assay is positive, the sample is reflexed to a RPR assay, which, if positive, is reported with a titer and is indicative of active or recent syphilis infection. If the RPR is negative, the sample is reflexed to a second treponemal assay, such as the *T pallidum* particle agglutination (TP-PA) assay. If the TP-PA is positive, this would indicate previously treated or late-stage syphilis infection. Alternatively, if the TP-PA is negative, the initial positive screen is interpreted as a false positive result.

Syphilis screening at CHI Health Laboratory is performed by using the reverse algorithm, which first tests sera for *T pallidum* specific IgG/IgM antibodies using an automated MFI. A positive treponemal test suggests infection with *T pallidum* but does not distinguish between recent, past, treated or untreated infections. This is because treponemal tests may remain reactive for life, even following adequate therapy. Therefore, the results of a nontreponemal assay, such as RPR, are needed to provide information on a patient's disease state and history of therapy.(Table)

In some patients, the results of the treponemal screening test and RPR may be discordant (eg, syphilis IgG/IgM positive and RPR negative). To discriminate between a falsely reactive screening result and past syphilis, a second treponemal-specific antibody test is recommended using a method that is different from the initial screen test (eg, TP-PA).

### Guide to Syphilis Reverse Screening Interpretation

1) Result of 1 <sup>st</sup> treponemal test <b>Syphilis Screen</b> (multiplex flow immunoassay)	2) Result of Non-treponemal RPR (Rapid Plasma Reagin)	3) Result of 2 <sup>nd</sup> treponemal test <b>TP-PA</b> (Treponema Pallidum by Particle Agglutination)	<b>Interpretation</b>
Nonreactive	n/a	n/a	No serological evidence of infection. No further testing required, unless clinically indicated. Early or incubating syphilis infection cannot be excluded.
Reactive or Equivocal	Reactive	n/a	Presumptive evidence of infection. Likely untreated or recently treated syphilis. Follow CDC treatment guidelines.
Reactive or Equivocal	nonreactive	Reactive	Possible syphilis (eg, early or latent), or past, successfully treated syphilis. Thorough historical and clinical evaluation required.
Reactive or Equivocal	nonreactive	nonreactive	Likely false-positive screening test. No further testing required, unless clinically indicated.

### Limitations:

- Test results should be considered with other laboratory results, as well as the clinical presentation of the patient.
- A Nonreactive Syphilis Screen test does not exclude the possibility of exposure to or infection with *T. pallidum*. Antibodies may be low or undetectable levels in incubating or early primary disease and in some clinical conditions. Therefore results must be interpreted with caution.
- Detections of treponemal antibodies may indicate recent, past or successfully treated syphilis infections are therefore cannot be used to differentiate between active and cured cases.
- Circulating antibodies against yaws, pinta and bejel may interfere with syphilis screen assay (Bioplex Syphilis Total MFI).

\*\* CDC guidelines available at <https://www.cdc.gov/std/treatment-guidelines/syphilis.htm>